# Accumark Labs

# CERTIFICATE OF ANALYSIS

Paramount

| | |
|---|---|
| SAMPLE NAME: | CJC-1295 (no DAC) |
| SAMPLE CODE: | 43WZ-4ETW |
| RECEIVED DATE: | 07/20/2026 |
| PUBLISHED DATE: | 07/22/2026 |




| | |
|---|---|
| DECLARED IDENTITY | CJC-1295 (no DAC) |
| MATRIX TYPE: | PEPTIDE |
| SAMPLE NAME: | CJC-1295 (no DAC) |
| SAMPLE SIZE: | 10.0 mg |
| Nº LOT CODE: | 26VCJC171 |

**7.99 mg**
Total Quantity

**99.608%**
Total Blend Purity

| Sample | Test | Specification | Result | Status |
|---|---|---|---|---|
| CJC-1295 (no DAC) | IDENTITY | CJC-1295 (no DAC) | CJC-1295 (no DAC) | CONFORMS |
| CJC-1295 (no DAC) | QUANTITY | MEASURE | 7.99 mg | MEASURED |
| CJC-1295 (no DAC) | PURITY | > 98.0% | 99.608% | CONFORMS |

## HPLC Chromatogram Report

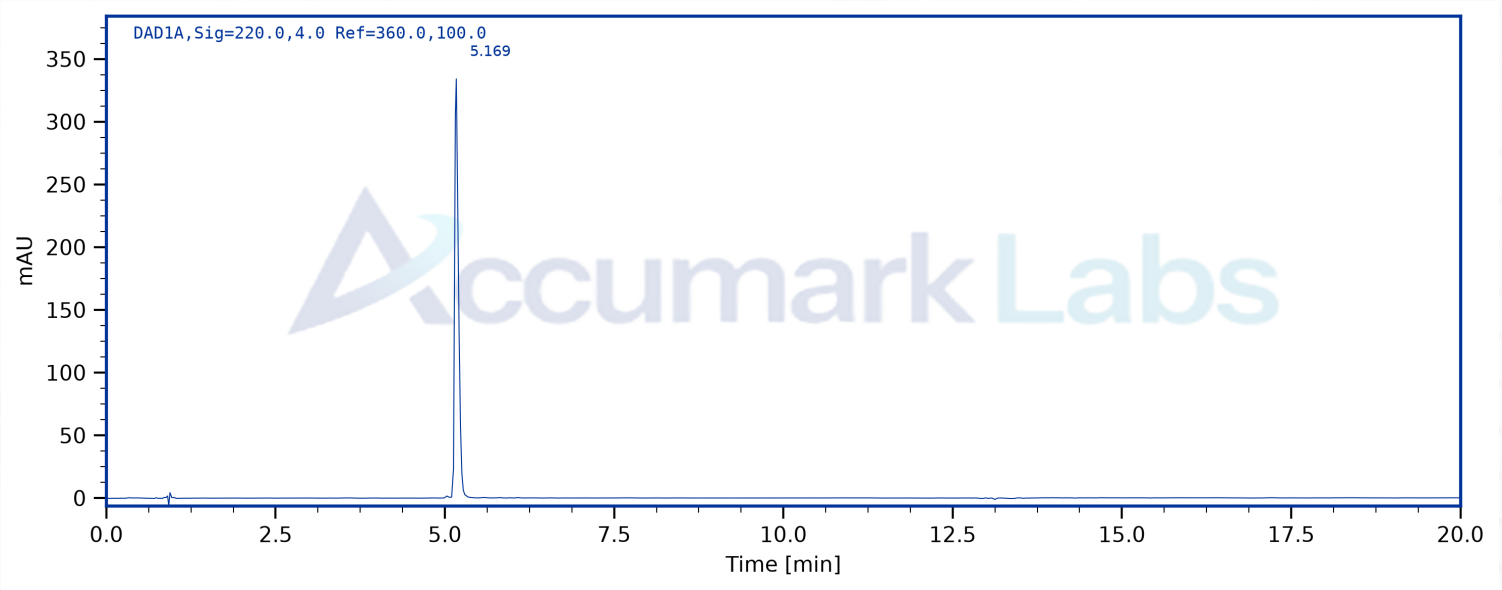


RESULTS REVIEWED BY:

Anthony Burke PhD
Lab Manager
07/22/2026

RESULTS CERTIFIED BY:

Dr. Levi Fried MD
Lab Director
07/22/2026

ACCUMARKLABS.COM
43WZ-4ETW
07/22/2026

# Accumark Labs

# CERTIFICATE OF ANALYSIS

Paramount

| | |
|---|---|
| SAMPLE NAME: | CJC-1295 (no DAC) |
| SAMPLE CODE: | 43WZ-4ETW |
| RECEIVED DATE: | 07/20/2026 |
| PUBLISHED DATE: | 07/22/2026 |

| Sample | Test | Specification | Result | Status |
|---|---|---|---|---|
| CJC-1295 (no DAC) | Endotoxin (LAL) | ≤ 5.0 EU/mL | Pass | CONFORMS |
| CJC-1295 (no DAC) | Rapid Sterility Screening (PCR) | Not Detected | Pass | CONFORMS |

RESULTS CERTIFIED BY:

Anthony Burke PhD
Lab Manager
07/22/2026

RESULTS CERTIFIED BY:

Dr. Levi Fried MD
Lab Director
07/22/2026

ACCUMARKLABS.COM
43WZ-4ETW
07/22/2026